

University of Groningen

## The use of biodegradable fixation devices in the treatment of osteochondritis dissecans and osteochondral fractures

Wouters, Diederick Bernard

**IMPORTANT NOTE:** You are advised to consult the publisher's version (publisher's PDF) if you wish to cite from it. Please check the document version below.

*Document Version*

Publisher's PDF, also known as Version of record

*Publication date:*  
2009

[Link to publication in University of Groningen/UMCG research database](#)

*Citation for published version (APA):*

Wouters, D. B. (2009). *The use of biodegradable fixation devices in the treatment of osteochondritis dissecans and osteochondral fractures: fiction, future, fact.* [Thesis fully internal (DIV), University of Groningen]. [s.n.].

### Copyright

Other than for strictly personal use, it is not permitted to download or to forward/distribute the text or part of it without the consent of the author(s) and/or copyright holder(s), unless the work is under an open content license (like Creative Commons).

The publication may also be distributed here under the terms of Article 25fa of the Dutch Copyright Act, indicated by the "Taverne" license. More information can be found on the University of Groningen website: <https://www.rug.nl/library/open-access/self-archiving-pure/taverne-amendment>.

### Take-down policy

If you believe that this document breaches copyright please contact us providing details, and we will remove access to the work immediately and investigate your claim.

Downloaded from the University of Groningen/UMCG research database (Pure): <http://www.rug.nl/research/portal>. For technical reasons the number of authors shown on this cover page is limited to 10 maximum.

# CHAPTER 6

## **Is the pull-out force of the Meniscus Arrow® in bone affected by the inward curling of the barbs during biodegradation? An in vitro study.**

***D.B. Wouters<sup>1,3</sup>***

***J.G.M. Burgerhof<sup>2</sup>***

***R.R.M. Bos<sup>3</sup>***

***J.Th.M. de Hosson<sup>4</sup>***

<sup>1</sup> Department of General-, Arthroscopic Surgery and Traumatology,  
TweeSteden Hospital, Tilburg, The Netherlands,

<sup>2</sup> Department of epidemiology,  
University Medical Centre Groningen, Groningen, The Netherlands,

<sup>3</sup> Department of Oral and Maxillofacial Surgery,  
University Medical Centre Groningen, Groningen, The Netherlands,

<sup>4</sup> Department of Applied Physics,  
University of Groningen, The Netherlands.

## ABSTRACT

**Background:** Inward curling of the barbs of Meniscus Arrows during degradation was observed in a previous study, in which swelling, distention, and water uptake by Meniscus Arrows was evaluated. This change of configuration could have consequences with respect to anchorage capacity in bone.

**Material/Methods:** Eight non-degraded Meniscus Arrows in the original configuration were pulled out of thawed, fresh-frozen human femoral condyle, and pull-out force was measured and compared with that of 6 Meniscus Arrows after 31 days of degradation under controlled conditions.

**Results:** No significant difference was found between the 2 groups with respect to the required pull-out force (t test), the distribution of the data, or the interaction between degradation and location, as evaluated by Mann-Whitney test, and no significant difference was found between the 2 groups with respect to the degradation state or position in the condyles, as evaluated by 2-way analysis of variance.

**Conclusions:** Our results indicate that the decrease in barb-barb diameter during the first month of degradation of the Meniscus Arrows has no significant effect on the tensile pull-out force required for removal from human femur condyle. Further research should be undertaken to examine whether the same is true for other biodegradable devices with barbs.

## BACKGROUND

Metallic fixation devices such as screws,<sup>1,2</sup> pins<sup>3-5</sup> and staples<sup>6</sup> are generally used to fix small bony fragments in fracture treatment. Most require a second procedure for removal. When inserted into joints, removal is, in most circumstances, obligatory to prevent damage of the opposing cartilage. Even when embedded under the cartilage surface, protrusion can occur.<sup>7,8</sup> Removal prevents scattering during computed tomography or magnetic resonance imaging and also prevents localized tissue reaction<sup>9-11</sup>

The use of biodegradable devices obviates the need for removal and researchers have spent the last three decades in the development of appropriate materials and devices.

At present, different biodegradable polymers, such as polydioxanone, polyglycolic acid, and polylactic acid and their co-polymers, combinations or blends are available. Biodegradable screws or pins are applied for small fragment fixation in fracture treatment or treatment of osteochondritis dissecans. Screws and pins have specific advantages and disadvantages. Biodegradable screws produce the required compression, but their current minimal head diameter of 3 mm is considerable for the often fragile fragments. In addition, at least 2 devices are necessary to achieve rotational stability. Furthermore, during the degradation process, wear of the opposing cartilage and local tissue reactions can occur.<sup>12,13</sup> Biodegradable pins do not share these disadvantages, but do not provide compression.<sup>14,15</sup>

The Meniscus Arrows (MA; (ConMed Linvatec Ltd, Tampere, Finland) is a biodegradable nail-like device composed of L-DL(80/20) self-reinforced lactide copolymer with a very small core diameter (1.0mm), barbs and a small, flat head (Figure 1). Originally designed to mend ruptured menisci, the anchorage of MA's in bone was examined in previous *in vitro* study to evaluate the potential application in fixing small cartilage-bone fragments in the treatment of osteochondritis dissecans and small fragment fracture surgery<sup>16</sup> Theoretically, biodegradable polymers swell during degradation, which could prove an additional advantage for the use of biodegradable implants in fracture fixation. Their hold in bone would increase like an expanding bolt. For gels this distention


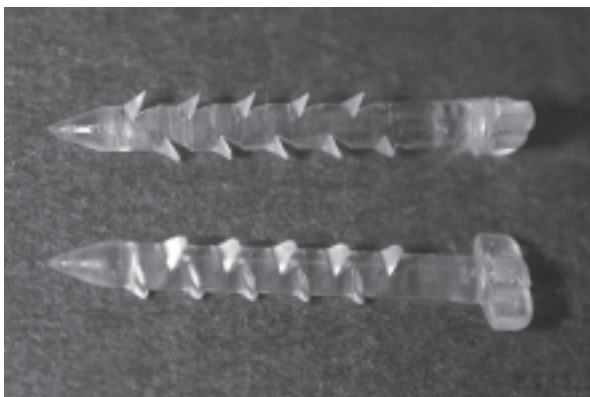


Figure 1: the Meniscus Arrow®


is variable<sup>17-21</sup> and we found that the swelling of MA's is negligible with respect to this mechanical aspect.<sup>22</sup> In the same study we observed consistent inward curling of the barbs of all MA's during the degradation process (Figure 2).<sup>22</sup> This phenomenon could result in a decreased hold in bone. Therefore, the aim of the present study was to evaluate the potential influence of this inward curling of the barbs on the required pull-out force from the bone.

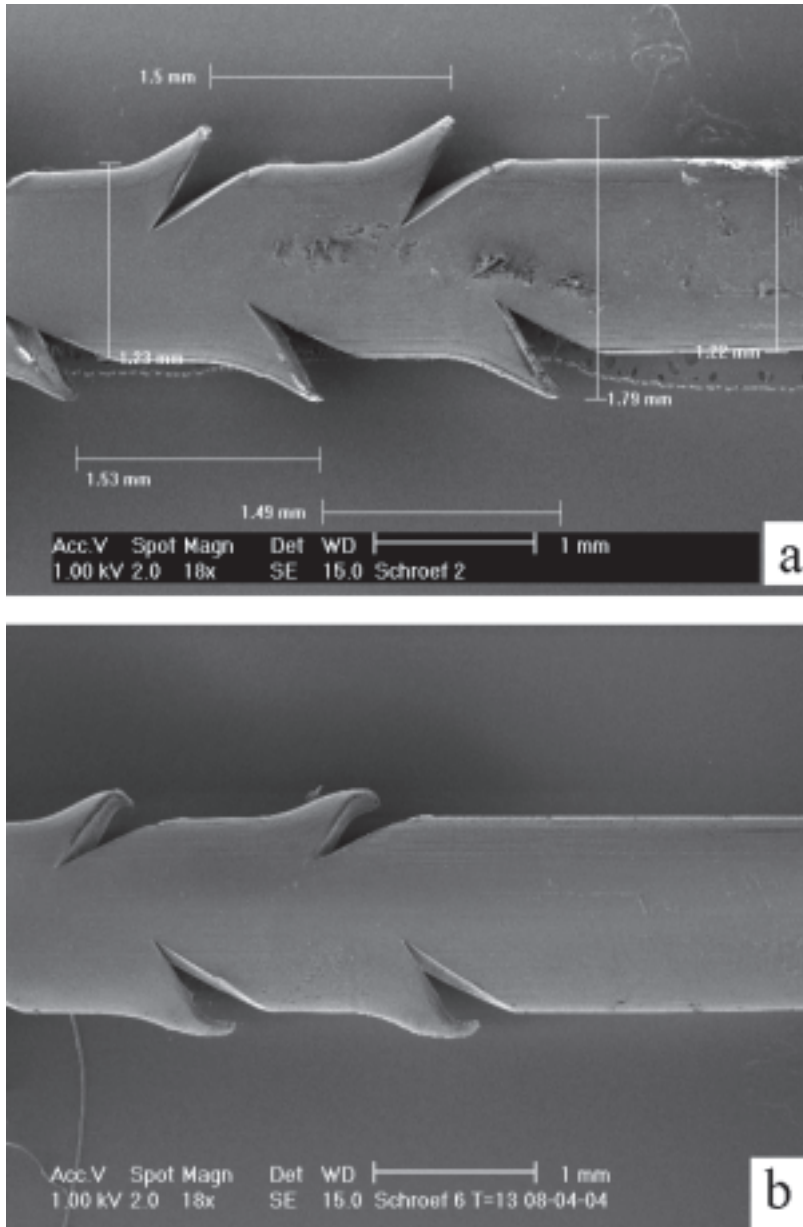


**Figure 2:** a: a non degraded Meniscus Arrow®  
b: after 31 days of immersion in a sterile saline solution

## MATERIAL AND METHODS

Group 1 (non- degraded MA's) consisted of eight MA's, retrieved directly from the packing. In group 2 (degraded MA's), six MA's were submerged over a period of 31 days in a sterile phosphate buffered saline (Pharmacy of the University Medical Centre, Groningen, The Netherlands) at 37° C. The solution was changed twice a week under sterile conditions. A degradation period of 31 days was selected because this period is the expected initial consolidation time for small fragment fractures in humans.

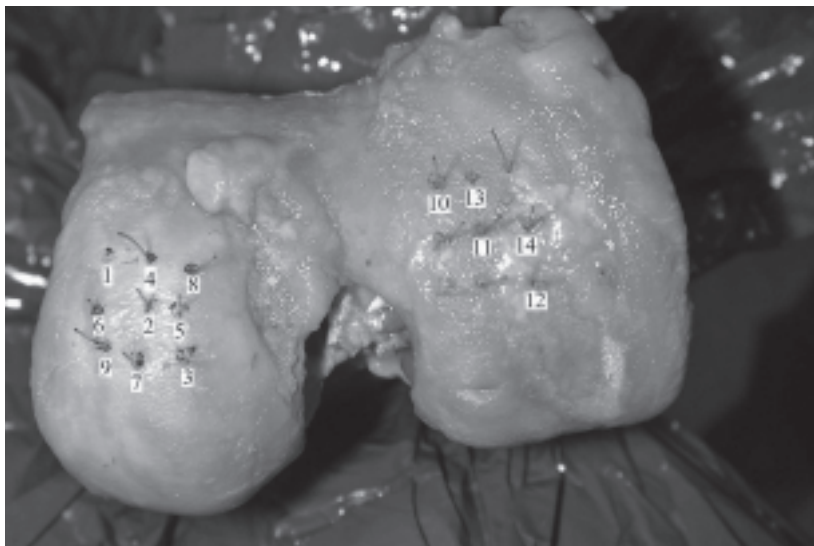

**Figure 3:** sequence of pulling out from the femur condyles. (see for color image: page 142)

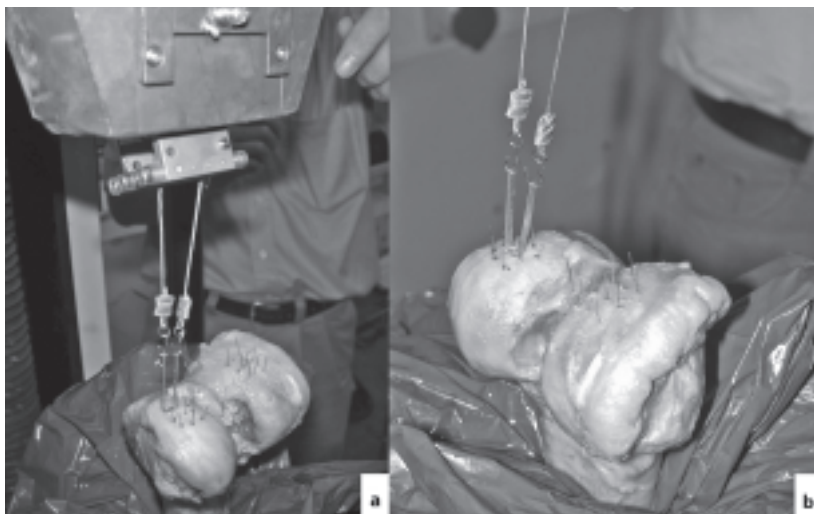

**Figure 4:** a: start of the extraction of the first Meniscus Arrow® from hole 1  
b: start of the extraction of the second Meniscus Arrow® from hole 2  
(see for color image: page 142)

For the experiment, 18 holes of 1.0mm in diameter were drilled into both condyles of a thawed, previously fresh frozen human cadaver femur, to exclude the influence of potential differences of local bone density (Figure 3). Alternating non-degraded and degraded MA's, were then via a hole in an extracting device and gently hammered into each drill hole (Figure 4a). Standard hand-insertion instruments were used. The MA's were subsequently pulled out, using an Instron 1195 draw bench (Instron, 825 University Ave. Norwood, MA 02062-2643, USA). The load cell measured 1000newtons (N) maximum, with a scale set at 0N – 200N. The extraction speed applied to the device was 5mm / min.

### Statistical analysis

The results were statistically analyzed by *t*-test, Mann-Whitney test and 2-way analysis of variance.

## RESULTS

In group 1, the peak required pull-out force of the eight non-degraded MA's ranged from 12.82N to 41.19 N with an average  $\pm$ standard deviation of  $28.61\text{N} \pm 11.17$  (table 1). In group 2, the required pull-out force for degraded MA's ranged of 12.80N to 34.22N, with an average of  $21.83\text{N} \pm 7.63\text{N}$ .

The average extraction force of the new, non-degraded MA's and the degraded MA's did not differ significantly (*t*-test:  $P = .23$ , 95% confidence interval for the difference in means: [ - 4.8 ; 18.4]). In addition, the spread of the results did not differ significantly (Leven's test  $P = .16$ ). Results of 2-way analysis of variance showed no significant difference between degradation and location ( $P = .7$ ), between degraded or non-degraded MA's ( $P = .15$ ) or between location on the lateral- in the lateral or medial condyle ( $P = .14$ ).

## DISCUSSION

The use of biodegradable devices is advantageous if the fixation lasts long enough to allow for consolidation with minimal damage to the fixed bony fragments and if the degradation occurs without adverse effects.

The Meniscus Arrow is one such potential fixation device,<sup>14,15,22</sup> but the inward curling of the barbs, encountered in our previous study<sup>22</sup> could lead to decreased anchorage in the bone over time. We found no other reports describing this curling or its potential effect on the hold of MA's or other biodegradable devices. This provided the impetus for the present study.

Although the inward curling of the barbs after a degradation period of 31 days suggests that this could lead to a decrease of the anchorage to a solid material such as bone, this is not confirmed in the present study. Therefore, this phenomenon does not appear to interfere with the application of MA's in fixing small bony fragments in fracture surgery or in osteochondritis dissecans.

## **CONCLUSIONS**

The inward curling of the barbs of MA's during degradation did not affect the anchorage in bone in our tests.

Whether other biodegradable devices with barb-like restraints deform spontaneously during degradation as will require additional research.



## References

1. Cugat R, Garcia M, Cusco X, Monllau JC, Vilario J, Juan X, Ruiz-Cotorro A. Osteochondritis Dissecans: A historical Review and its Treatment with cannulated screws. *Arthroscopy* 1993;9(6):675–684
2. Mackie IG, Pemberton DJ, Maheson M. Arthroscopic use of the Herbert screw in osteochondritis dissecans. *J Bone Joint Surg* 1990;72B:1076
3. Smillie IS. Treatment of osteochondritis dissecans. *J Bone Joint Surg (B)* 1957;39: 248–260
4. Anderson A, Lipscomb AB, Coulam C. Antegrade curettement, bone grafting and pinning of osteochondritis dissecans in the skeletally mature knee. *Am J Sports Med* 1990;18(3):254–261
5. Guhl JF. Arthroscopic treatment of Osteochondritis Dissecans. *Clin Orth* 1982;167:65–74
6. Kivistö R, Pasanen L, Leppilahti J, Jalovaara P. Arthroscopic repair of osteochondritis dissecans of the femoral condyles with metal staple fixation: a report of 28 cases. *Knee Surg Sports Traumatol Arthrosc* 2002;10:305 – 309
7. Bobic V. Cover photograph, *Arthroscopy* 2001;17(5)
8. Kivistö R, Pasanen L, Leppilahti J, Jalovaara P. Arthroscopic repair of osteochondritis dissecans of the femoral condyles with metal staple fixation: a report of 28 cases. *Knee Surg Sports Traumatol Arthrosc* 2002;10:305 – 309
9. Scher N, Poe D, Kuchmir F, Reft C, Weichselbaum R, Panje WR. Radiotherapy of the resected mandible following stainless steel plate fixation. *Laryngoscope* 1988;98:61–563
10. Castillo MH, Button TM, Homs MI, Pruett CW, Doerr R. Effects of radiation therapy on mandibular reconstruction plates. In: *Trans 41<sup>st</sup> Ann Cancer Symp. The Society of Surgical Oncology, New Orleans, Louisiana, U.S.A. 1988; 144*
11. Black J. *Orthopedic Biomaterials in Research and Practice.* Churchill Livingstone New York, Edinburgh London, Melbourne 1988; p 292–302
12. Kumar A, Malhan K and Roberts SNJ. Chondral Injury from Bioabsorbable Screws after Meniscal Repair. *Arthroscopy* 2001;17(8):34
13. Friederichs MG, Greis PE, Burks RT. Pitfalls associated with fixation of Osteochondritis Dissecans fragments using bioabsorbable screws. *Arthroscopy* 2001;17(5):542–546
14. Weckström M, Parviainen M, Kiuru MJ, Mattila VM, Pihlajamäki HK. Comparison of Bioabsorbable Pins and Nails in the Fixation of Adult Osteochondritis Dissecans fragments of the Knee: an Outcome of 30 Knees. *Am J Sports Med* 2007;35(9):1467-1477
15. Wouters DB, Bos RRM, van Luyn MJA. “Should in the treatment of Osteochondritis Dissecans biodegradable or metallic fixation devices be used? A comparative study in goat knees.” *J Biomed Mater Res B Appl Biomater.* 2008 Jan;84(1):154–164
16. Wouters DB, Bos RRM, Mouton LJ, van Horn JR. The Meniscus Arrow® or metal screw for treatment of Osteochondritis dissecans? In Vitro comparison of their effectiveness. *Knee Surg Sports Traumatol Arthrosc* 2004;12:52–57
17. Hasirci V, Lewandrowski K, Gresser JD, Wise DL, Trantolo DJ. Versatility of biodegradable biopolymers: degradability and an in vivo application. *J Biotechnol* 2001 30;86(2):135-50
18. Pego AP, Van Luyn MJ, Brouwer LA, van Wachem PB, Poot AA, Grijpma DW, Feijen J. In vivo behavior of poly(1,3-trimethylene carbonate) and copolymers of 1,3-trimethylene carbonate with D,L-lactide or epsilon-caprolactone: Degradation and tissue response. *J Biomed Mater Res.* 2003 Dec 1;67A(3):1044–1054
19. Bergsma EJ, de Bruijn WC, Rozema FR, Bos RRM, Boering G. Late degradation tissue response to poly(L-lactide) bone plates and screws. *Biomaterials.* 1995;16(1):25–32
20. Wang DA, Williams CG, Li Q, Sharma B, Elisseff JH. Synthesis and characterization of a novel degradable phosphate-containing hydrogel. *Biomaterials* 2003;24(22):3969–3980

21. Shin H, Quinten Ruhe P, Mikos AG, Jansen JA. In vivo bone and soft tissue response to injectable, biodegradable oligo(poly(ethylene glycol) fumarate hydrogels. *Biomaterials* 2003;24(19):3201–3211
22. Wouters DB, Bos RRM, De Hosson JTh.. Swelling of solid biodegradable implants during degradation. An in-vitro study with Meniscus Arrows®. *Knee Surg Sports Traumatol Arthrosc* 2007;15:1204–1209

